



Learn More About
iScreen OFD Employee Drug Testing Kits
EmployeeDrugTestingAce.com
 Trusted Proven Secure
www.DrugTestingAce.com www.EDTAce.com

Oral Fluid Drug Screen

A Rapid Screening Test.

- Integrated Testing Solution
- Five and Six Panel Configurations Offered
- Simple Procedure

Innovative Drug Screening Solutions
Quality • Choices • Support

For Forensic Use Only

Instant Technologies, Inc.



an  inverness medical company

iScreen™ OFD

Oral Fluid Drug Screen A Rapid Screening Test.

Introducing an all-new saliva collection device, the iScreen™ OFD.



iScreen™ OFD
6-panel shown as a negative result.

Drug Name:	Abbr:	Cutoff:
Amphetamine.....	AMP.....	50ng/ml
Methamphetamine.....	mAMP.....	50ng/ml
Marijuana.....	THC.....	12ng/ml
Phencyclidine.....	PCP.....	10ng/ml
Cocaine.....	COC.....	20ng/ml
Opiates.....	OPI.....	40ng/ml




Configurations:

- 4-panel...I-DSB-745-021.....COC, THC, OPI, mAMP
- 5-panel...I-DSB-755-011.....COC, THC, OPI, mAMP, AMP
- 6-panel...I-DSB-765-011.....COC, THC, OPI, mAMP, AMP, PCP

Receive a free DVD system complete with an iScreen OFD training video on an initial order of four boxes of iScreen OFD's.

Procedure Card

For Forensic Use Only

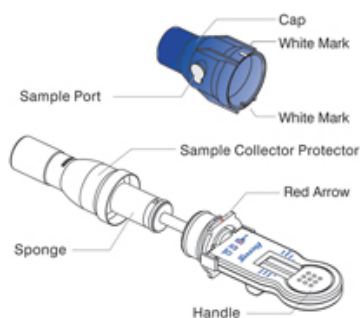


Section I: Sample Collection

- Instruct the donor not to place anything in the mouth including food, drink, gum or tobacco products for at least 10 minutes prior to collection.
- Remove Sample Collector Protector.
- Insert Sponge end of collector into mouth. Actively swab the inside of the mouth and tongue with Sponge. As soon as the Sponge softens slightly, gently press the Sponge between the tongue and teeth to ensure **complete saturation**. The Sponge is saturated when no hard spots can be felt. Collect for at least three (3) minutes before removing Sponge. Hand the saturated collector over to the tester.




Section II: Testing

- Align the Red Arrow on the device with either one of the White Marks on the Cap. Insert the collector vertically into the Cap and press down firmly until the Cap reaches the thread.
 - Twist the Handle clockwise 180° to tighten the Cap until the Red Arrow lines up with the other White Mark.
 - Place the test device horizontally on a clean and level surface with facing up.

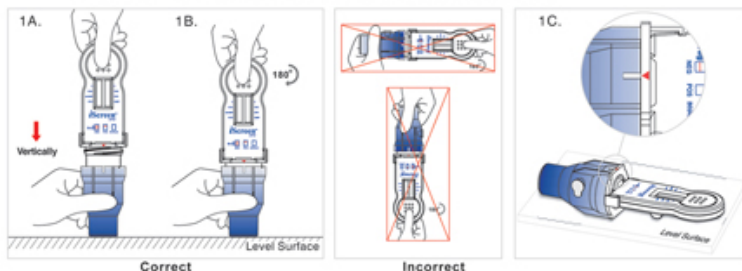

- Read results at five (5) minutes. Results stable up to sixty (60) minutes.



* All positive results are presumptive and should be confirmed by an alternate method. The preferred confirmatory method is GC/MS or GC/MS/MS.

- If results are positive, secure Cap with Security Seal and send to laboratory for confirmation.

